

# R&S® Spectrum Rider FPH Release Notes

## Firmware Version V2.60

These Release Notes are for following models of R&S® Spectrum Rider FPH:

R&S®FPH02,	order no. 1321.1111.02,	order no. 1321.1111.52,
R&S®FPH06,	order no. 1321.1111.06,	order no. 1321.1111.56,
R&S®FPH13,	order no. 1321.1111.13,	order no. 1321.1111.63,
R&S®FPH26,	order no. 1321.1111.26,	order no. 1321.1111.76,
R&S®FPH23,	order no. 1321.1711.23,	
R&S®FPH36,	order no. 1321.1711.36,	
R&S®FPH44,	order no. 1321.1711.44,	
R&S®FPH54,	order no. 1321.1711.54	

© 2024 Rohde & Schwarz GmbH & Co. KG  
Muehldorfstr. 15, 81671 Munich, Germany  
Phone: +49 89 41 29 - 0  
E-mail: [info@rohde-schwarz.com](mailto:info@rohde-schwarz.com)  
Internet: <http://www.rohde-schwarz.com>

Subject to change – Data without tolerance limits is not binding.  
R&S® is a registered trademark of Rohde & Schwarz GmbH & Co. KG.  
Trade names are trademarks of the owners.

1320.8893.00 | Version 15 | R&S® Spectrum Rider FPH |

The software makes use of several valuable open source software packages. For information, see the "Open Source Acknowledgment" provided with the product.

PAD-TM: 3574\_32886.02/08.0008.00/CI/1/EN

**ROHDE & SCHWARZ**  
Make ideas real



# Contents

<b>1</b>	<b>Information on the current version and history .....</b>	<b>3</b>
1.1	New functions .....	3
1.2	Modified functionality.....	5
1.3	Improvements .....	6
1.4	Known issues.....	8
<b>2</b>	<b>Modifications to the documentation .....</b>	<b>9</b>
<b>3</b>	<b>Firmware update .....</b>	<b>10</b>
<b>4</b>	<b>Firmware Options .....</b>	<b>12</b>
<b>5</b>	<b>Customer support.....</b>	<b>13</b>

# 1 Information on the current version and history

## 1.1 New functions

The following table lists the new functions and indicates the version in which the new function was introduced:

### New functions in firmware V2.60:

Version	Improvements
V2.60	Quick Naming Support in File Browser
V2.60	Support for Isotropic antenna TS-EMF-B2E

### New functions in earlier firmware versions:

Version	Functions
V2.50	Support for R&S®NRPxxP Pulse Power Sensor. Requires option R&S®FPH-K29
V2.40	Supports reset of "Max Hold" Trace in Spectrum Analyzer Mode
V2.40	Added steps for Compass Calibration for HE400 Antenna under Antenna Service Menu
V2.40	Display measured power value in Occupied Bandwidth Measurement Mode
V2.30	Supports EMF Measurement Application. Requires Option R&S®FPH-K105
V2.20	Support of new instrument models: R&S® FPH 5kHz to 13.6 GHz with tracking generator, order no. 1321.1711.23 R&S® FPH 5kHz to 26.5 GHz with tracking generator, order no. 1321.1711.36 R&S® FPH 5kHz to 44.0 GHz, order no. 1321.1711.44 R&S® FPH 5kHz to 44.0 GHz with tracking generator, order no. 1321.1711.54
V2.10	Added SCPI Commands to retrieve compass information obtained by FPH from HE400 antenna
V2.10	Added SCPI Commands to retrieve GPS time obtained by FPH from the connected GPS mouse
V2.10	Support for HE800-PA antenna in variant FPH .26
V2.10	Included ICNIRP Limit lines to default files in FPH
V2.00	Supports Gated Trigger Measurements in SEM, ACLR and OBW Measurement modes. Requires Option R&S®FPH-K57
V2.00	Support for saving dataset in csv format (in Spectrum Analyzer mode only)
V2.00	Support for explicit Horizontal and Vertical polarization in EIRP measurements

<b>V2.00</b>	Added SCPI Command to read out Memory Trace
<b>V1.90</b>	Support of Marker Tracking in Spectrum Analyzer Application
<b>V1.90</b>	EIRP measurement mode
<b>V1.80</b>	Gated Trigger Support for Channel Power Measurement, Spectrogram and Spectrogram playback applications
<b>V1.80</b>	Spectrum Analyzer frequency extension from 5 kHz down to 100 Hz for FPH models .06/.13/.26. Requires R&S®FPH-B29
<b>V1.80</b>	Audio tone function added to Spectrum Analyzer Application
<b>V1.70</b>	Support of digital demodulation (ASK/FSK) - requires R&S®FPH-K7
<b>V1.70</b>	Support for N-Type Connector in model R&S®FPH26 (Only at production in the factory) - requires R&S®FPH-B100
<b>V1.70</b>	High resolution frequency counter (up to 0.001 Hz)
<b>V1.70</b>	Support of additional Power Meter units Vemf, dBuVemf, dBmVemf
<b>V1.60</b>	Frequency extension up to 31 GHz (available on specific FPH variants)
<b>V1.60</b>	Instrument Sanitization/Secure Flash Erase
<b>V1.60</b>	Support of optical power sensor UPM100 from ODM Inc. (works with K9-Option)
<b>V1.60</b>	Modulation Rate display in FM Demodulation (works with K7-Option)
<b>V1.60</b>	Support for HE400BC and HE400MW Antenna
<b>V1.50</b>	Support for Gated Sweep
<b>V1.50</b>	Support for HE400 Antenna
<b>V1.50</b>	Support for Trigger Delay in Video Trigger
<b>V1.50</b>	Support for NRP6 and NRP6AN Power Sensors (only via USB interface)
<b>V1.40</b>	Isotropic Antenna support for R&S®FPH-K43: Receiver Mode
<b>V1.40</b>	Advanced Measurement Modes: OBW (Occupied Bandwidth), TDMA Power, SEM (Spectrum Emission Mask), ACLR (Adjacent Channel Leakage Ratio), Harmonic Distortion, AM Modulation Depth
<b>V1.40</b>	Display Line for Spectrum Analyzer
<b>V1.40</b>	Device Power ON after Power Restored Configurable
<b>V1.40</b>	R&S®FPH-K16: Signal Strength Mapping Tone feature
<b>V1.30</b>	R&S®FPH-K43: Receiver Mode
<b>V1.30</b>	R&S®FPH-K15: Interference Analysis
<b>V1.30</b>	R&S®FPH-K16: Signal Strength Mapping
<b>V1.30</b>	Isotropic Antenna for Spectrum Analyzer Mode

V1.30	Save on Event for Spectrum Analyzer, Maps and Receiver Mode
V1.30	Channel Power Measurement in Spectrum Analyzer Mode
V1.30	Transducers and dBuV unit support in Power Meter
V1.30	New gestures for File Preview, skip Wizard Measurement step
V1.30	New gestures hide/show Info-Bar in Spectrum Analyzer and Receiver Mode
V1.30	Support for Yagi antennas HA-Z901 and HA-Z1900 (New Transducer files)
V1.20	R&S®FPH-K7: Analog Modulation Analysis
V1.20	Wizard
V1.20	Marker audio demodulation in zero span
V1.20	Multiple languages: Support of 12 languages in user interface
V1.20	GPS: Support of R&S®HA-Z340
V1.20	Disable and enable the touchscreen
V1.20	File browser user interface improvement
V1.20	Instrument- View: Support of remote display
V1.10	R&S®FPH-K9: Power Sensor Support
V1.10	R&S®FPH-K19: Channel Power Meter
V1.10	R&S®FPH-K29: Pulse Measurements with Power Sensors
V1.10	Marker: Added move marker position from touchscreen
V1.10	File Manager: Added Recall-Screenshot preview function
V1.10	Color Themes: Added Black & White and Printer Friendly UI themes

## 1.2 Modified functionality

The following table lists the modified functions and indicates the version in which the modification was carried out:

### Modified functionality in firmware V2.60:

None

### Modified functionality in earlier firmware versions:

Version	Functions
V2.50	Support added for R&S HA-Z340 GPS receiver accessory variant

V2.40	Following improvements done in EMF measurement application (Requires Option R&S®FPH-K105) - Displays the remaining time to complete the ongoing EMF Measurement - Default Unit is changed to dBuV/m
V2.30	Default location for saving datasets upon pressing the screenshot button is changed to the folder named 'dataset'
V2.20	Maps Application (R&S®FPH-K16): Indoor Position button is enabled only when a USB thumb drive is plugged in.
V2.10	Maximum possible Sweep time in Spectrum Analyzer for zero span increased to 3000s
V2.10	Speed improvements for FFT computation in Spectrum Analysis Application
V2.10	Sweep Time calculations adjusted for better accuracy
V2.10	Maps Application: Indoor Position is now enabled even when USB thumb drive is not plugged in
V2.00	Boot up screen is updated
V2.00	Improved Booting time (roughly 2 seconds)
V2.00	Improved Spur performance
V1.90	SNR added to Analog Modulation Summary View
V1.90	Support of HE400MW Antenna
V1.90	Supports automatic reboot after firmware update from InstrumentView
V1.80	Improved display of Power Level in Channel Power Measurement to two decimal point accuracy
V1.80	Trace View Mode selection for Trace 2 in Spectrum Analyzer application
V1.80	SCPI command to turn on high resolution frequency counter
V1.80	Dataset and screen shot saving to non-default working directory
V1.60	Channel Power Measurement in Maps
V1.50	Smooth and faster Navigation in File Browser and in Setup Pages
V1.40	R&S®FPH-K43: Receiver Mode 10.000 point support
V1.40	R&S®FPH-K43: Receiver Mode RMS and Average detector support for longer measurement times

### 1.3 Improvements

The following tables list the improvements and indicate since which version these improvements are available:

#### Improvements in firmware V2.60:

Version	Improvements
V2.60	Improved Spur performance
V2.60	LO unlock could occur at certain frequencies. This issue is fixed
V2.60	Video trigger issues could occur for sweep time < 300ms. These issues are fixed

#### Improvements in earlier firmware versions:

Version	Improvements
V2.50	Fixed issue of randomly showing up HE400-NO MODULE or HE400-UNKNOWN and automatic saving of GPS positions in Maps Application when HE400 antenna is connected.
V2.50	Fixed shadow signal in the trace observed at a specific center frequency
V2.50	Improved Spur performance
V2.40	Improved spur performance
V2.40	Fixed Azimuth value not displayed in Triangulation mode when HE400MW antenna was used
V2.40	Fix missing trace at certain configurations when Isotropic Antenna is enabled
V2.33	Improved noise floor level behavior at lower frequencies in variants R&S®FPH06 R&S®FPH13 and R&S®FPH26
V2.32	Spikes and dips could occur at certain frequencies in variant FPH.26 when RMS or sample detector is enabled. This issue is fixed.
V2.31	Fix issue in installing Option R&S®FPH-B29 in models model's R&S®FPH.23, R&S®FPH.36, R&S®FPH.44 and R&S®FPH.54
V2.30	Sweep time Improvements with Tracking generator turned ON (Applicable only to models R&S®FPH.23, R&S®FPH.36 and R&S®FPH.54)
V2.20	Corrected the Trace average calculation in Receiver Mode Application (R&S®FPH-K43)
V2.00	With Option R&S®FPH-B29 installed, the displayed Frequency extension value in Installed Options Page is corrected to 100Hz
V1.90	Fixed Command [SENSE:]SWEep:POINTs? In Spectrum Analyzer Mode
V1.90	Fixed issue where MAC address is not visible when device is turned-on with no network cable connected
V1.90	Missing parameters for K-29 Pulse Power Measurements are enabled back
V1.80	Improved spurious performance in FPH models .06/.13/.26
V1.70	Improvement in (faster) detection of Power Sensors
V1.70	Improved synthesizer settings in R&S®FPH26
V1.50	Improved Measurement Speed

<b>V1.40</b>	R&S®FPH-K43: Receiver Mode improved scan startup time for scans with large number of points
<b>V1.40</b>	Fix for GPS number of satellites always showing 12
<b>V1.20</b>	Fixed device unable to restart if date is 2002 or earlier
<b>V1.10</b>	Localization: Chinese translations were improved

## 1.4 Known issues

<b>Version</b>	<b>Improvements</b>
<b>V2.50</b>	FPH device should be powered on before plugging in the R&S®HA-Z340 GPS receiver



## 2 Modifications to the documentation

The latest manual from the R&S®Spectrum Rider FPH can be downloaded from the product web page at <http://www.rohde-schwarz.com/manual/fph>.

## 3 Firmware update

New firmware versions usually contain new features, improvements of existing functionality, bug fixes etc. When a new firmware version is available, it is recommended to replace the old firmware with the new one.

### R&S®InstrumentView

Firmware release V2.60 corresponds to R&S®InstrumentView V3.3, which is available on the Rohde & Schwarz web page as a separate update package.

Although older versions of R&S®InstrumentView might be able to communicate with firmware release V2.60, an update of R&S®InstrumentView is highly recommended, as older R&S®InstrumentView versions might not support all functions included in the new firmware release.

### Updating the firmware

The latest firmware version is available for download on the internet:

<http://www.rohde-schwarz.com/firmware/fph>



Before you update the firmware, you should make a backup of the data that you have stored on the R&S®Spectrum Rider FPH (datasets, screenshots, transducer factors etc.). You can make a backup with the tools available in the R&S®InstrumentView software package. The firmware update itself does not delete or modify that data, but it is recommended to perform a factory reset after the firmware update to update predefined limit lines, channel tables etc. The factory reset, however, does delete user data.

1. Download the firmware installer from the internet.  
The firmware comes in a single `.exe` file.
2. Save the file to the root directory of a memory stick.
3. Run the `.exe` file to unpack the self-extracting zip archive.


The following files are extracted.

```
FPH_<version>_bootloader_1.bin  
FPH_<version>_bootloader_2.bin  
FPH_<version>_bootloader_7.bin  
FPH_<version>_osimage.bin  
FPH_<version>_updater.bin  
FPH_<version>_xmegaloadfiles.bin
```

Make sure that only these files are present in the root directory of the memory stick.

4. Turn off the R&S®Spectrum Rider FPH Spectrum Analyzer.
5. Connect the memory stick to one of the USB interfaces of the R&S®Spectrum Rider FPH.

6. Press the "Preset" key and the number "8" key simultaneously.

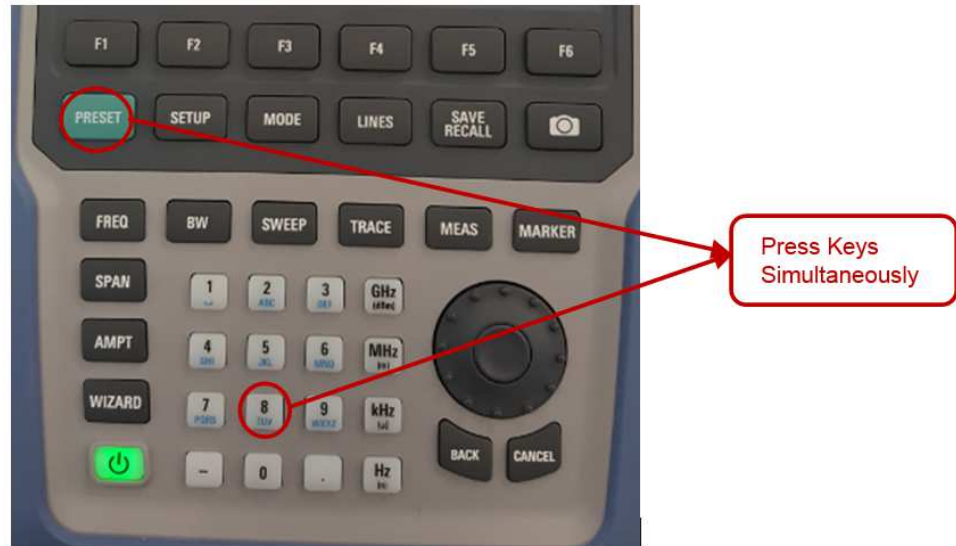

7. Turn on the R&S®Spectrum Rider FPH and keep pressing the two keys for at least 5 seconds after the startup screen appears.

8. Release the keys.

The booting process continues. After a couple of seconds, the R&S®Spectrum Rider FPH asks you if you really want to update the firmware.

9. Press the "Enter" (Round button in the rotary) key to update the firmware. (You can cancel the firmware update with the "CANCEL" key.)

The firmware update takes several minutes. The R&S®Spectrum Rider FPH shows a message when the firmware update is done.

**Note:** Do not turn off the R&S®Spectrum Rider FPH during the firmware update.

10. Turn off the R&S®Spectrum Rider FPH.

11. Turn on the R&S®Spectrum Rider FPH.

The R&S®Spectrum Rider FPH boots with the new firmware version.

12. Optional: It is recommended to perform a **factory reset** after a firmware update to replace the predefined limit lines, channel tables and other data with the latest updates.

**Note:** Before you start a factory reset, make sure to make a backup of your data that you have saved on the R&S®Spectrum Rider FPH. Otherwise that data is deleted.

## 4 Firmware Options

You can equip the R&S®Spectrum Rider FPH with optional functionality or firmware options like the analog demodulation application or the receiver application. These firmware options expand the functionality of the R&S®Spectrum Rider FPH with new measurement functions settings etc.

### Installing firmware options

To install a new firmware option, you have to enter a license key for validation.

The license key is included in the delivery of the firmware option.

1. Press the "Setup" key to enter the instrument setup menu.
2. Select the "Installed Options" menu item.  
The R&S®Spectrum Rider FPH shows a list of all options that are currently installed on your R&S®Spectrum Rider FPH.
3. Select the "Install Option" button and press the "Enter" key.  
The R&S®Spectrum Rider FPH opens an input field.
4. Enter the license key with the alphanumeric keys and confirm the entry with the "Enter" key.
5. The license key is a 30-digit number.

The R&S®Spectrum Rider FPH confirms a successful installation.

If the R&S®Spectrum Rider FPH shows an "Invalid Key Code" message, try to enter the license key again.

## 5 Customer support

### Technical support – where and when you need it

For quick, expert help with any Rohde & Schwarz product, contact our customer support center. A team of highly qualified engineers provides support and works with you to find a solution to your query on any aspect of the operation, programming or applications of Rohde & Schwarz products.

### Contact information:

Contact our customer support center at [www.rohde-schwarz.com/support](http://www.rohde-schwarz.com/support) or follow this QR code:



Figure 5-1: QR code to the Rohde & Schwarz support page.